

X-Rays

Jan Kybic

2005–2013

Overview

- ▶ Fundamentals of X-rays
- ▶ Generation of X-rays
- ▶ Detection of X-rays
- ▶ Imaging and diagnostic methods

Invention



1895, W. Röntgen



B. Röntgen hand



modern hand

Electromagnetic spectrum

Electromagnetic wave spectrum

Energy (eV)	Frequency (Hz)		Wavelength (m)
4×10^{-11}	10^4	AM radio waves	10^4
4×10^{-10}	10^5		10^3
4×10^{-9}	10^6		10^2
4×10^{-8}	10^7		10^1
4×10^{-7}	10^8	Short radio waves FM radio waves and TV	10^0
4×10^{-6}	10^9		10^{-1}
4×10^{-5}	10^{10}	Microwaves and radar	10^{-2}
4×10^{-4}	10^{11}		10^{-3}
4×10^{-3}	10^{12}	Infrared light	10^{-4}
4×10^{-2}	10^{13}		10^{-5}
4×10^{-1}	10^{14}	Visible light	10^{-6}
4×10^0	10^{15}		10^{-7}
4×10^1	10^{16}	Ultraviolet light	10^{-8}
4×10^2	10^{17}		10^{-9}
4×10^3	10^{18}	X-ray	10^{-10}
4×10^4	10^{19}		10^{-11}
4×10^5	10^{20}		10^{-12}
4×10^6	10^{21}		10^{-13}
4×10^7	10^{22}	Gamma ray	10^{-14}
		Cosmic ray	

Particles and waves

- ▶ reflection, scattering, refraction, diffraction
- ▶ photons with energy $E = hf$,
 $\lambda = 1 \text{ nm} \approx 1.2 \cdot 10^3 \text{ eV} = 1.2 \text{ keV}$
- ▶ ionizing radiation (above 1 eV)

Chest X-rays radiography machine



Chest X-ray



X-ray scanner







FIGURE 1.1. (Left) The basic setup for X-ray imaging. The collimator restricts the beam of X-rays so as to irradiate only the region of interest. The antiscatter grid increases tissue contrast by reducing the number of detected X-rays that have been scattered by tissue. (Right) A typical planar X-ray radiograph of the chest, in which the highly attenuating regions of bone appear white.

X-ray source

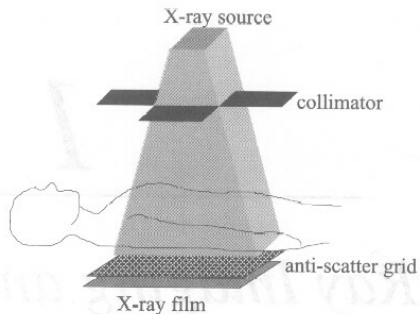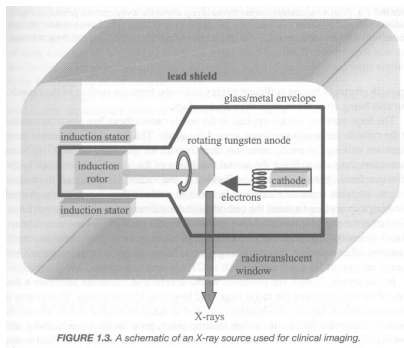


- ▶ 15 ~ 150 kV, rectified AC
- ▶ 50 ~ 400 mA anode current
- ▶ tungsten wire (200 μm) cathode, heated to $\sim 2200^\circ\text{C}$
- ▶ anode rotates at 3000 rpm
- ▶ molybdenum or tungsten-rhenium anode
- ▶ thermoionic emission

Beam focusing

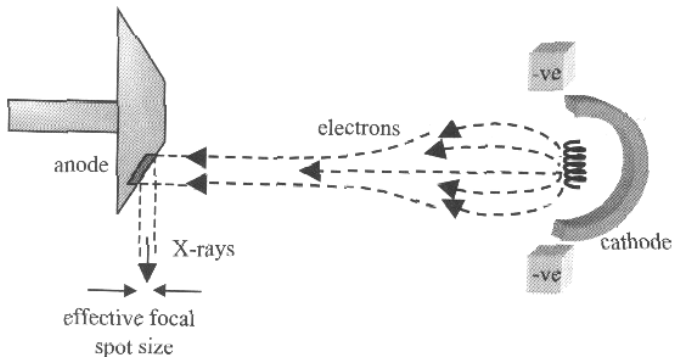


- ▶ Focal spot size 0.3 mm ~ 1.2 mm

Penumbra

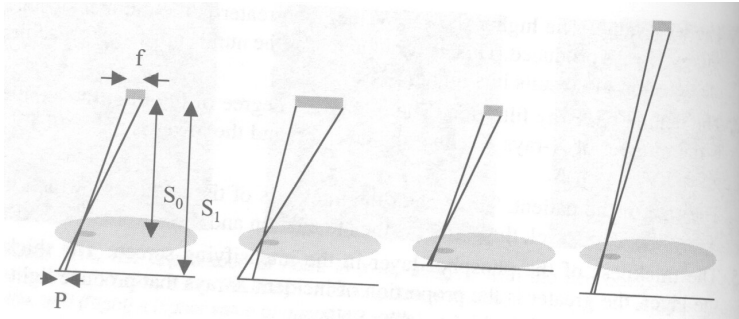

- ▶ geometric unsharpness
- ▶ small focal spot
- ▶ large distance


X-ray tube

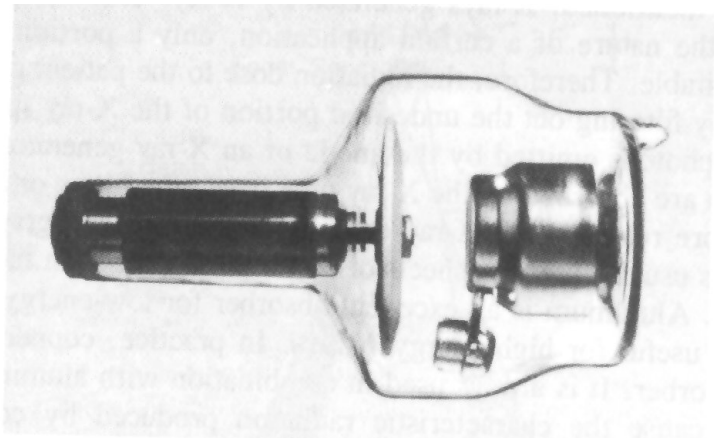

X-ray parameters

Intensity: [W/m^2]: $\propto U^2 I$

Spectrum: (150 kV)

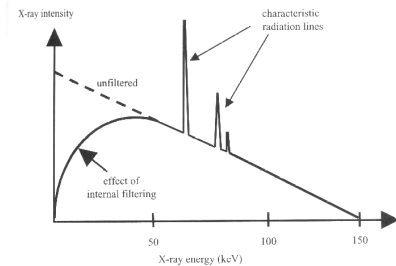


- ▶ Bremsstrahlung
- ▶ Characteristic radiation
- ▶ Filter low-energy rays that would not penetrate the patient — Al sheets. (skin dose reduced $80\times$)

Interaction between X-rays and matter


- ▶ Coherent scattering
- ▶ Photoelectric effect
- ▶ Compton scattering
- ▶ (*Pair production*)
- ▶ (*Photodisintegration*)

Coherent (Rayleigh) scattering

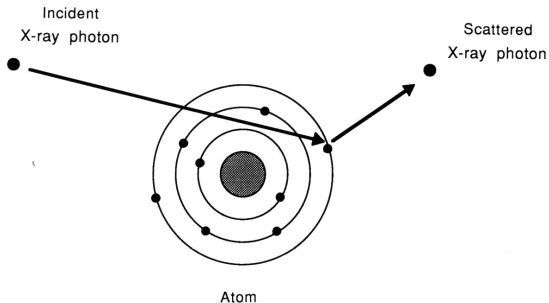


- ▶ Photon \longrightarrow photon
- ▶ Low-energy radiation
- ▶ Probability $\propto Z_{\text{eff}}^{8/3} / E^2$.
 - ▶ Z_{eff} - effective atomic number
 - ▶ muscle $Z_{\text{eff}} \approx 7.4$, bone $Z_{\text{eff}} \approx 20$
- ▶ About 5 ~ 10 % of tissue interactions

Photoelectric effect

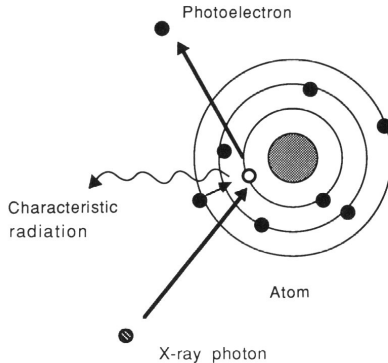


- ▶ High-energy radiation
- ▶ Photon \rightarrow characteristic radiation, photo-electron / Auger electron, positive ion
- ▶ \rightarrow ionization
- ▶ Desirable, X-ray photon completely absorbed

Photoelectric interaction wrt E

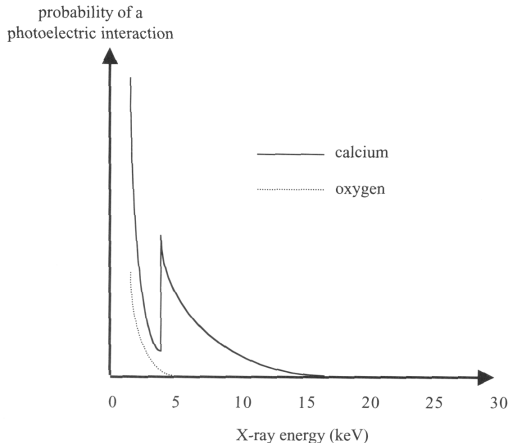

- ▶ K -edge
- ▶ Probability $\propto Z_{\text{eff}}^3/E^3$ (above K -edge)
- ▶ Excellent contrast bone/tissue at low E

Compton scattering

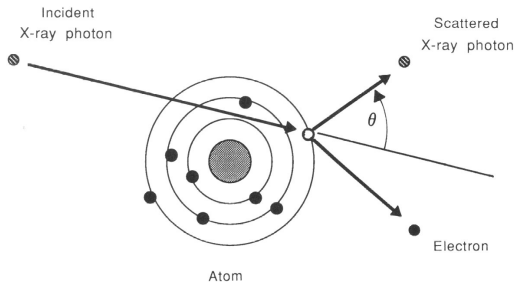

$$E_{\text{scatt}} = \frac{E_{\text{inc}}}{1 + \frac{E_{\text{inc}}}{m_e c^2} (1 - \cos \theta)}$$

- ▶ photon \rightarrow photon + electron, ionization
- ▶ most frequent in X-ray imaging, especially for high E_{inc}
- ▶ independent to atomic number \rightarrow small contrast
- ▶ background noise, health hazard

Attenuation

$$dI = -n\sigma I dx$$

$$I_x = I_0 e^{-\mu x}$$

μ — linear attenuation coefficient

Half-value layer $\approx 0.693/\mu$

TABLE 1.2. The Half-Value Layer (HVL) for Muscle and Bone as a Function of the Energy of the Incident X-Rays


X-ray energy (keV)	HVL, muscle (cm)	HVL, bone (cm)
30	1.8	0.4
50	3.0	1.2
100	3.9	2.3
150	4.5	2.8

Mass attenuation coefficient μ/ρ


Attenuation factors wrt E

$$\mu = \mu_{\text{photoel}} + \mu_{\text{Compton}} + \mu_{\text{coherent}}$$


Linear attenuation coefficient
(cm^{-1})

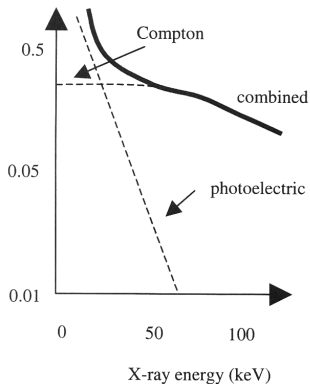


Mass attenuation coefficient
(cm^2g^{-1})

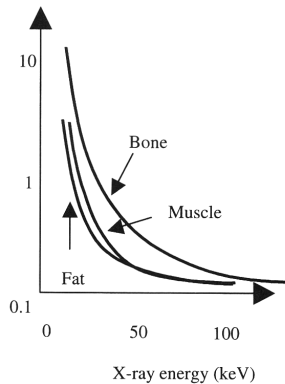


Attenuation wrt E (2)

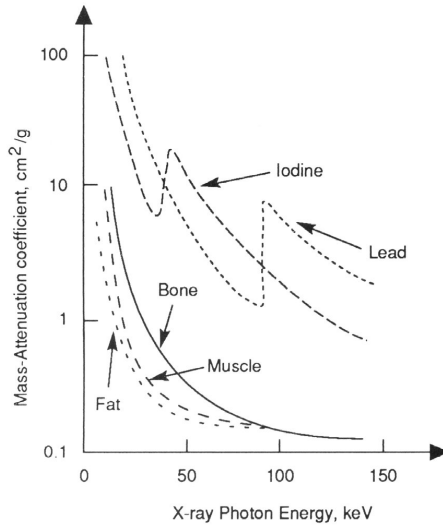


Effects of Compton scattering

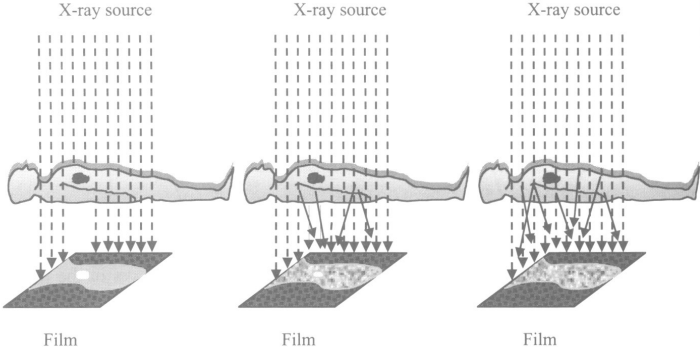



Beam restrictor / Collimator

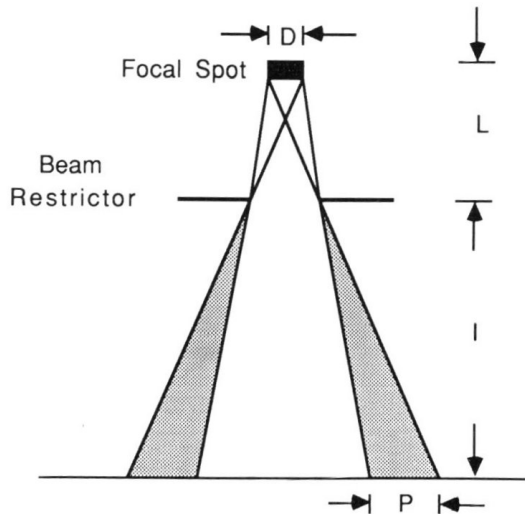

Beam restrictor / Collimator (2)


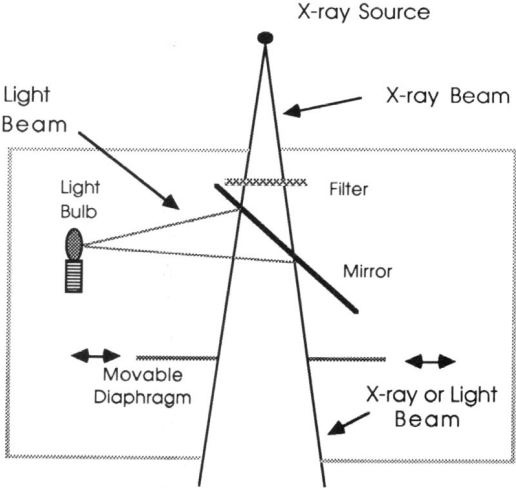


Antiscatter grid

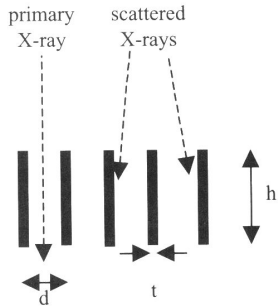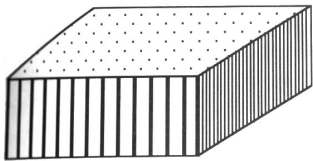

Bucky factor = efficiency



Intensifier screen

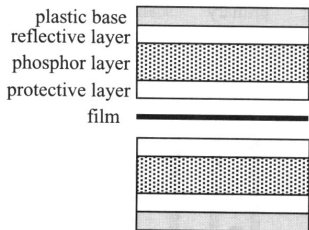

- ▶ 50× sensitivity increase
- ▶ thickness; trade-off resolution/sensitivity
- ▶ Gd — green, La — blue
- ▶ efficiency 20 %

Film

- ▶ monochromatic (sensitive to blue), orthochromatic (sens. to green)
- ▶ double emulsion ($10\ \mu\text{m}$), silver bromide in gelatin
- ▶ blackening, optical density (OD) $\log_{10}(I_i/I_t)$
- ▶ contrast $\gamma = \frac{OD_2 - OD_1}{\log_{10} E_2 - \log_{10} E_1}$, slope of the linear region
- ▶ latitude (dynamic range), range of useful exposure values
- ▶ grain size sensitivity/resolution trade-off
- ▶ mixed-particle size \rightarrow high contrast
- ▶ automatic exposure control, ionization chamber



Digital Sensors

- ▶ Computed radiography (CR)
 - ▶ Phosphor-based storage plate
 - ▶ chemical storage (oxidation of Eu)
 - ▶ laser scanning, light erasure


Digital Sensors

- ▶ Computed radiography (CR)
 - ▶ Phosphor-based storage plate
 - ▶ chemical storage (oxidation of Eu)
 - ▶ laser scanning, light erasure
- ▶ Digital radiography (DR)
 - ▶ flat-panel detectors (FPD)
 - ▶ thin-film transistor (TFT) array
 - ▶ CsI scintillator → photo-diode/transistor
 - ▶ 41×41 cm, 2048×2048 pixels
 - ▶ better dynamic range, quantum efficiency, and latitude wrt film

Digital Sensors

- ▶ Computed radiography (CR)
 - ▶ Phosphor-based storage plate
 - ▶ chemical storage (oxidation of Eu)
 - ▶ laser scanning, light erasure
- ▶ Digital radiography (DR)
 - ▶ flat-panel detectors (FPD)
 - ▶ thin-film transistor (TFT) array
 - ▶ CsI scintillator → photo-diode/transistor
 - ▶ 41×41 cm, 2048×2048 pixels
 - ▶ better dynamic range, quantum efficiency, and latitude wrt film
- ▶ Charge coupled device (CCD)
 - ▶ Phosphor screen, fiber-optic cables, CCD sensor
 - ▶ good sensitivity, low noise

X-ray image characteristics

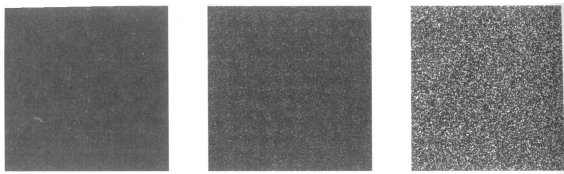

▶ Signal-to-noise ratio (SNR)

- ▶ Quantum mottle, source variation, Poisson distribution,
- ▶ $SNR \propto \sqrt{N}$, N — rays per area
- ▶ exposure time and current, $SNR \propto \sqrt{TI}$
- ▶ higher U \rightarrow more high-energy rays \rightarrow more incident rays \rightarrow better SNR
- ▶ X-ray filtering \rightarrow smaller SNR
- ▶ patient size, antiscatter grid, intensifying screen, film

X-ray image characteristics


- ▶ **Signal-to-noise ratio (SNR)**
- ▶ **Spatial resolution**
 - ▶ point spread function (PSF), line spread function (LSF), edge spread function (ESF), modulation transfer function (MTF)
 - ▶ thickness of the intensifier screen
 - ▶ speed of the X-ray film
 - ▶ geometric unsharpness
 - ▶ magnification factor (patient → film). Place patient as close as possible.

X-ray image characteristics


- ▶ **Signal-to-noise ratio (SNR)**
- ▶ **Spatial resolution**
- ▶ **Contrast-to-noise ratio**
 - ▶ $\text{CNR} = \frac{|S_A - S_B|}{\sigma_N} = |\text{SNR}_A - \text{SNR}_B|$

X-ray contrast agents

- ▶ barium sulfate, gastrointestinal tract

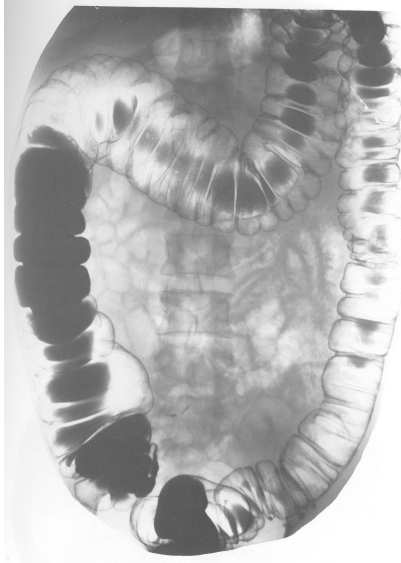

X-ray angiography

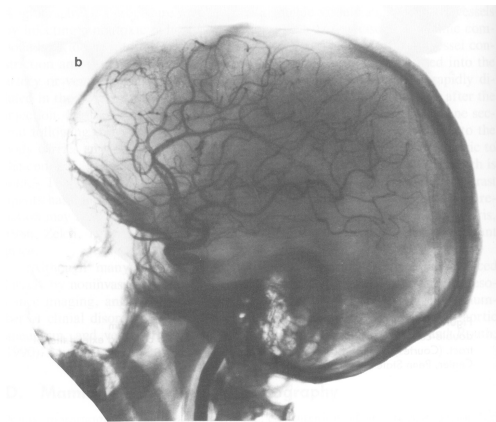


- ▶ Stenosis, clotting of arteries
- ▶ Iodine-based contrast agent
- ▶ Time series (*video*)

X-ray angiography


- ▶ Stenosis, clotting of arteries
- ▶ Iodine-based contrast agent
- ▶ Time series (*video*)
- ▶ Excellent resolution ($100\ \mu\text{m}$)
- ▶ Digital subtraction angiography
- ▶ Registration needed

Fluoroscopy / Intra-operative imaging

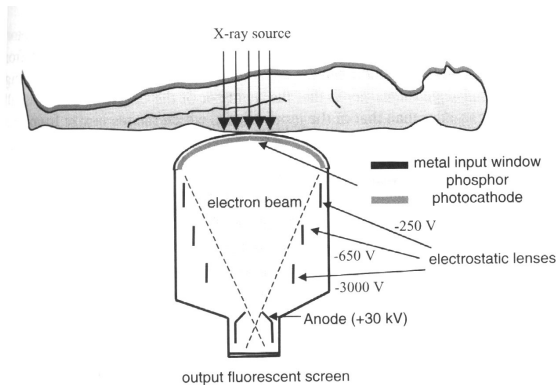

- ▶ Now a FPD/CCD instead of the fluorescent screen.

Dual-Energy Imaging

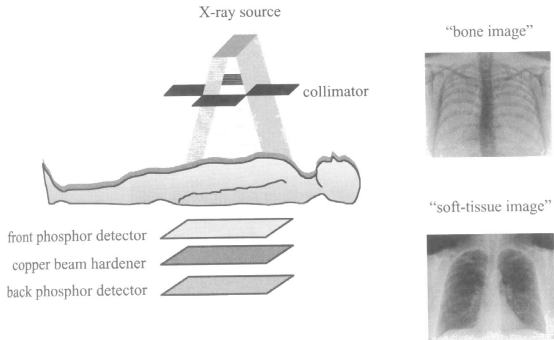

- ▶ Two exposures
- ▶ Two detectors
- ▶ Beam hardening

Mamography



- ▶ low U (25 ~ 30 kV), filter high-energy rays
- ▶ digital mamography, CCD sensor (1024 × 1024 pixels)

Advantages / disadvantages

- ▶ Advantages

- ▶ Widely used and available
- ▶ Experts available
- ▶ High-spatial resolution
- ▶ Excellent imaging of hard tissues (bones)

- ▶ Disadvantages

- ▶ Radiation exposure
- ▶ Difficulty in imaging soft-tissues
- ▶ 2D projection, hidden parts

New trends

- ▶ FPD/CCD sensors replace film
- ▶ higher sensitivity, faster exposure, lower dose
- ▶ dynamic imaging
- ▶ CT